

UniSeal®

**Vinyl
Powder-Free**



Synthetic Exam Gloves

Manufacturing Standards


Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	Level 11	1.5
Visual Defects (major)	S-4	1.5
Visual Defects (minor)	S-4	2.5
Dimensions	S-2	4.0

Physical Properties

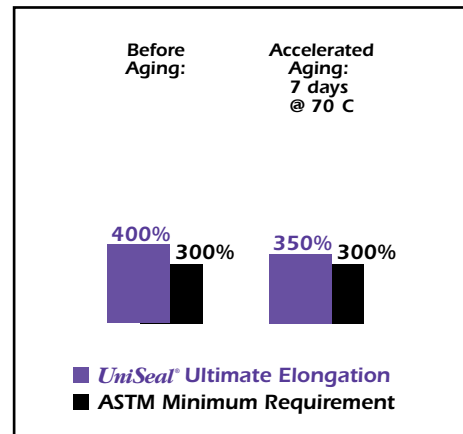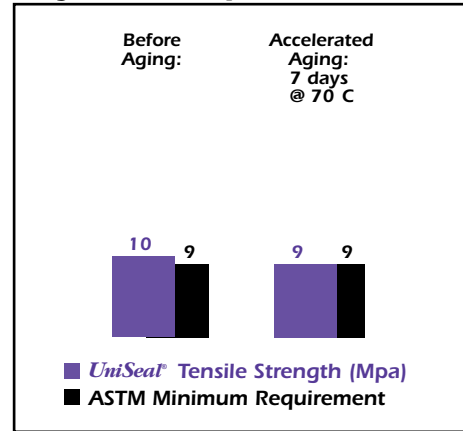

**S
P
E
C
S**



Sizes:	Item #:	
	Powdered:	Powder-Free:
XS	016-5	017-5
S	016-6	017-6
M	016-7	017-7
L	016-8	017-8
XL	016-9	017-9

9"
cuff

5
mil

CE **ISO 9002**

Quality Standards:

- Meets or exceeds the following standards:
ASTM D5250-00e4, D6124-01 (USA), EN 455 (EEC), AS 40 (Australia), FDA, CE
- Quality sampled in accordance with MIL.STD 105D
- ISO 9002 Certified Manufacturing

Dimensions (all measurements in mm)

Glove Length	Palm Width ±5mm	THICKNESS ±0.02mm		
		Cuff	Palm	Finger
240	75	0.09	0.12	0.14
240	85	0.09	0.12	0.14
240	95	0.09	0.12	0.14
240	105	0.09	0.12	0.14
240	115	0.09	0.12	0.14

Type: **Non-Sterile Examination Glove**
Shape: **Ambidextrous**