

UniSeal®

**Nitrile
Powder-Free**



**Textured
Synthetic Exam Gloves**

Manufacturing Standards


Brand new state-of-the-art manufacturing plant with computer-controlled market-leading technology.

Defect	Inspection Level	AQL
Pinholes (FDA 1000ml watertight test)	G1	1.5
Visual Defects (major)	G1	2.5
Visual Defects (minor)	G1	4.0
Dimensions	S-2	4.0

Physical Properties

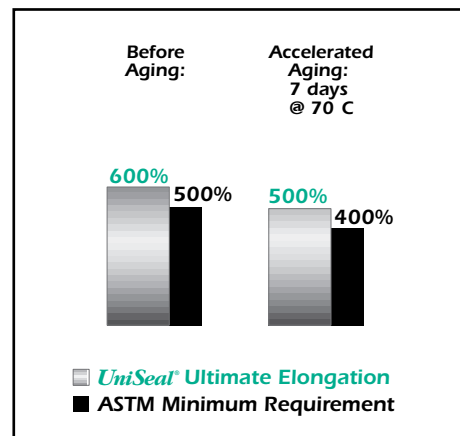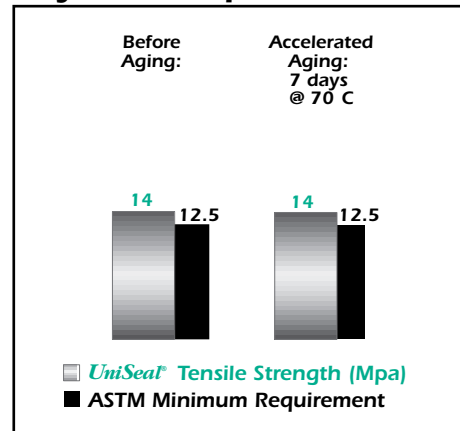

**S
P
E
C
S**



Sizes:	Item #:	
	Powdered:	Powder-Free:
S	093-6	094-6
M	093-7	094-7
L	093-8	094-8
XL	093-9	094-9

9"
cuff

4
mil



ISO 9001:2000

Quality Standards:

- Meets or exceeds the following standards:
ASTM D3578-00, ASTM D6124-00 (USA), EN 455 (EEC), AS 40 (Australia), FDA, CE, NFPA
- Quality sampled in accordance with MIL.STD 105D
- ISO 9001:2000 Certified Manufacturing

Dimensions (all measurements in mm)

Glove Length	Palm Width <small>±0.03mm</small>	THICKNESS <small>±0.03mm</small>		
		Cuff	Palm	Finger
(S)240	84	0.08	0.12	0.15
(M)240	94	0.08	0.12	0.15
(L)240	105	0.08	0.12	0.15
(XL)240	113	0.08	0.12	0.15

Type: Non-Sterile Examination Glove

Shape: Ambidextrous